



medemagroup



Serial number: _____

Delivery date: _____ Year 20_____

This vehicle was supplied by:

Date: /

Dealer:

For this product You can expect to find the following documentation:

- User manual
- Service manual
- Spare parts list
- pre-sale information.

Medema A/S

Enggårdvej 7
Snebjerg
DK - 7400 Herning

Phone: +45 70 10 17 55
Mail: info@medema.com

Contents

Contents	3
Intended occupant.....	5
Help for the visually impaired	5
FSN (Field Safety Notice).....	5
Symbols.....	6
Warning!	6
Joystick	6
Introduction.....	7
Flame resistance	8
Seat and backrest	8
Declaration of conformity	9
Medema A/S Warranty.....	10
Part names MC 1124 Spinalus-2.....	11
Part names MC 1124 - Spinalus.....	12
Introduction CJSM1.....	13
Designations - buttons.....	13
Symboles.....	13
Settings menu.....	15
Trouble shooting	19
Safety check.....	20
Programming	21
Serial number.....	22
Getting in and out of MC 1124.....	22
Driving the MC 1124	23
Brakes.....	27
Fuses	28
Batteries	29
Battery disposal.....	29
Charging.....	30
General care.....	31
Service intervals	31
Insurance.....	31
Storage	32
Transporting by motor vehicle.....	32
Securing to vehicle floor with belts	33
DAHL docking system	35
Mounting the docking spear.....	36
Public transport. (Train / bus).....	38
Transporting by plane	40
Towing	40
Changing the wheels.....	41
Checking the battery poles.....	45
Replacing batteries	45

Light.....	47
Lap belt.....	48
Footplate/footrest.....	49
Spinalus-2 settings.....	61
Stepless adjustment of seat depth	62
Height adjustment of armrest.....	63
Adjusting the headrest.....	68
Swing-away fitting for Spinalus-2.....	68
Adjusting the ION seat.....	73
Reconditioning	74
Returning electronic devices	75
Technical data.....	76
Seat angles.....	79

Intended occupant

The intended occupant of the wheelchair is a person with limited or no ability of working themselves.

The wheelchair is equipped with a joystick control which makes it usable for an occupant who only has functionality in the fingers. It can be driven with only one hand either left or right.

The occupant must be able to see in order to register traffic signals and other road users when driving in traffic. The occupant can be deaf and/or speechless.

The occupant must have a cognitive ability to understand the operation of the joystick and its buttons and icons.

The maximum occupant weight is 150 kg.

Help for the visually impaired

If you have difficulty reading small print in the user manual, we recommend that you visit our website, where you can read this manual in PDF format. You can enlarge the PDF manual on your PC monitor to suit your needs and preferences.

If you find it difficult to understand the manual and have general questions about the product, please feel free to contact us. You can find our contact info on page two in this user manual.

You can find manuals for all our products on our web page www.medema.dk. Or contact Medema A/S, and we can send the manuals in a mail for you. Find the contact information on page two in this manual.

FSN (Field Safety Notice)

All information concerning safety can be found at www.medema.com, which is always updated with the latest safety information. In the event of important safety-related changes, we will notify our customers directly (FSN).

Symbols



Used in the manual to indicate sections describing situations where extra care is required owing to the risk of personal injury.



Used to indicate sections on electromagnetic compatibility (EMC).

Warning!



For safety reasons the vehicle must not be lent to persons who are not completely familiar with it. The vehicle is designed for one person only.



The MC 1124 has been designed for persons weighing up to 150 kg.

Joystick



The joystick control box must not be exposed to extremes of temperature or kept in a damp environment for extended periods.



The joystick control box must not be subjected to heavy knocks.



Do not switch off the control box while driving, except in an emergency, as this may damage the electronics.



For cleaning, use a damp cloth with slightly soapy water. Do NOT allow any water or moisture to enter the control box.

Introduction

Congratulations on your new MC 1124 electric mobility wheelchair.

You are now the owner of an electric mobility wheelchair developed for use indoors as well as outdoors. It is what is called a Class B vehicle according to the European standard EN 12184.

To get the best out of this vehicle - and to avoid breakdowns and accidents - we recommend that you read this User Manual carefully. If you are a new user, you should pay particular attention to the section "Driving the MC 1124".

The MC 1124, and any assistive product are designed to stay safe to use for at least 10 years, up to a maximum of 5,000 hours, providing it has service and safety inspections every third year, which is equivalent to around 1500 operating hours. The service must be carried out either by Medema A/S or an authorised workshop.



IMPORTANT! For safety reasons it is of the utmost importance that service and safety check intervals are complied with, as this minimises the risk of brake failure and short-circuits in the wiring, which could generate heat and cause a fire.

We offer a wide range of accessories for the MC 1124 that can make everyday life easier for you. You are always welcome to contact us for further information on special accessories and adaptations.

Medema Production A/S is not responsible for any damage or injuries caused by inappropriate or unsafe use of the MC 1124.

If you have any further questions about the MC 1124 or this User Manual, you are always welcome to get in touch. Our contact details are as follows:

Medema A/S
Phone: +45 70 10 20 54
Email: info@medema.com
Internet: www.medema.dk

NB: Errors and omissions excepted. We reserve the right to update this manual as required.

Seat and backrest

The cover of the seat and backrest can be washed in the washing machine. ALWAYS follow the washing instructions on the back of the seat pad / backrest.



Flame resistance

The Mini Crosser seat's flame resistance has been tested in accordance with DS/ISO 7176-16:2013 Resistance to ignition of postural support devices.



Warning

The seat may become very hot if exposed to direct sunlight. Similarly, the seat will become very cold if it is exposed to cold temperatures, e.g., frost.

Medema A/S Warranty

1:

There is a 2-year warranty, with the exception of worn parts such as tires, hoses, fuses, light bulbs, bushings and brake pads.

2:

If you want to make a claim for a part under the warranty, it must be intact. The warranty will be void if the product has been removed or appears to have been mishandled.

3:

There is a 5-year warranty against breakage and corrosion of the undercarriage.

4:

For the warranty to cover batteries, the charger used must be sold by Medema A/S.

The fabric, type and serial number must be indicated on the warranty specification, otherwise, warranty coverage may be denied.

5:

Items returned under a warranty claim must be suitably packaged to prevent damage during transport. Items damaged during transport due to poor packaging will not be covered by the warranty.

6:


The warranty does not cover freight costs.

7:

The warranty requires inspection according to the intervals specified in the technical specifications. Service and maintenance must be carried out by Medema authorised professionals.


Part names MC 1124 Spinalus-2

The part names given below refer to the descriptions later in the instruction manual.

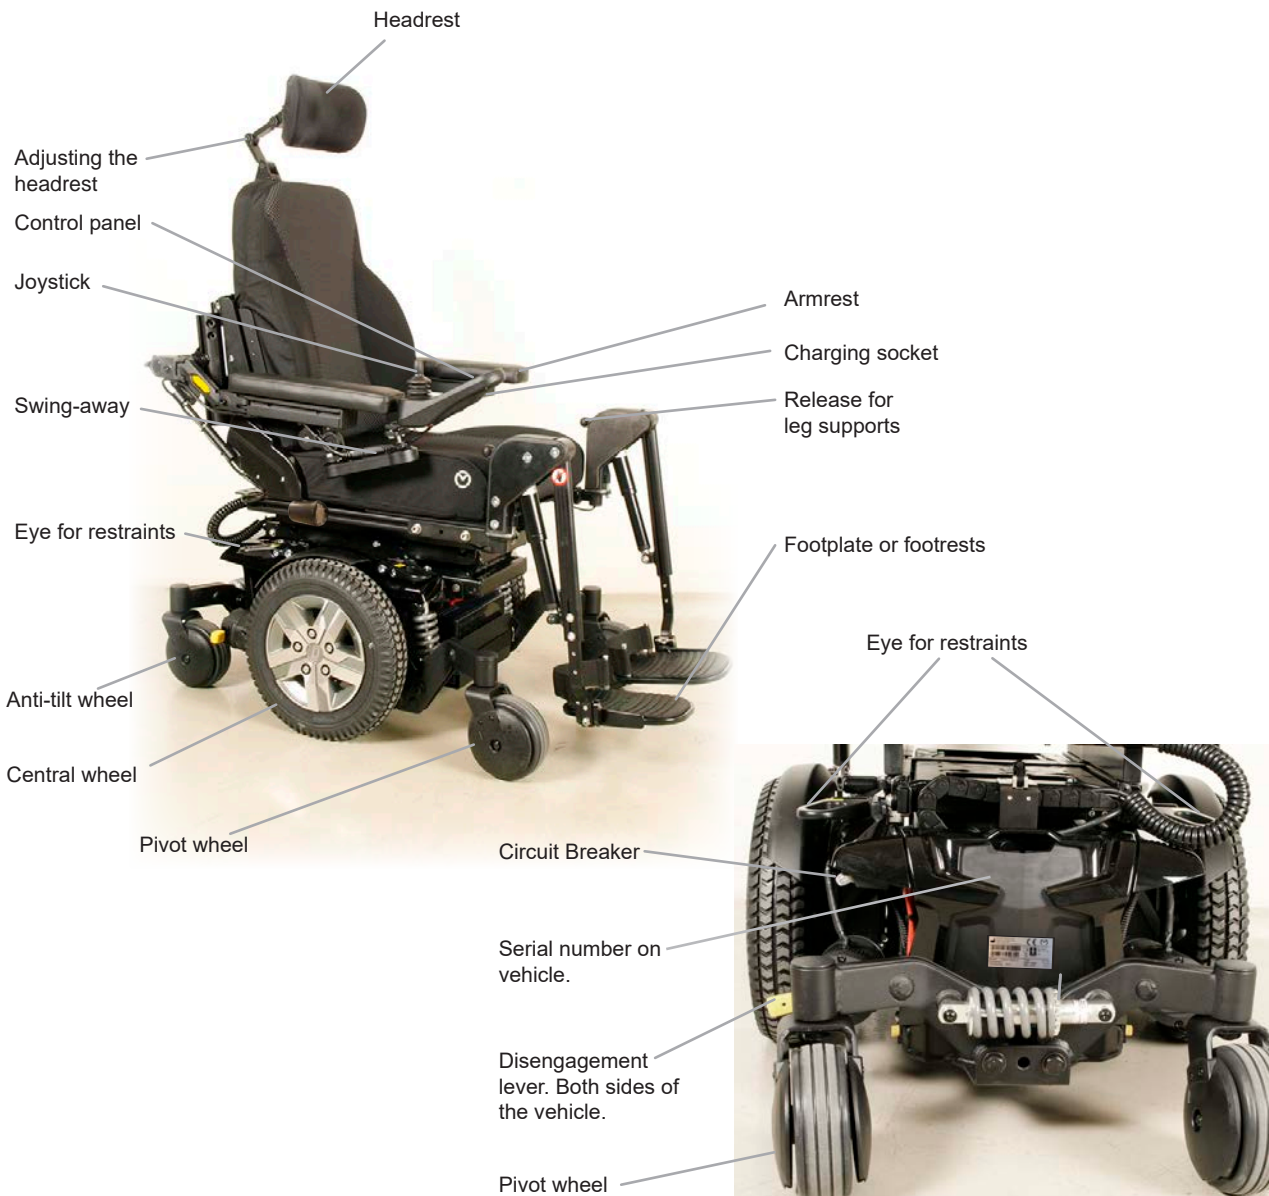

Part names MC 1124 - Spinalus

The part names given below refer to the descriptions later in the instruction manual.

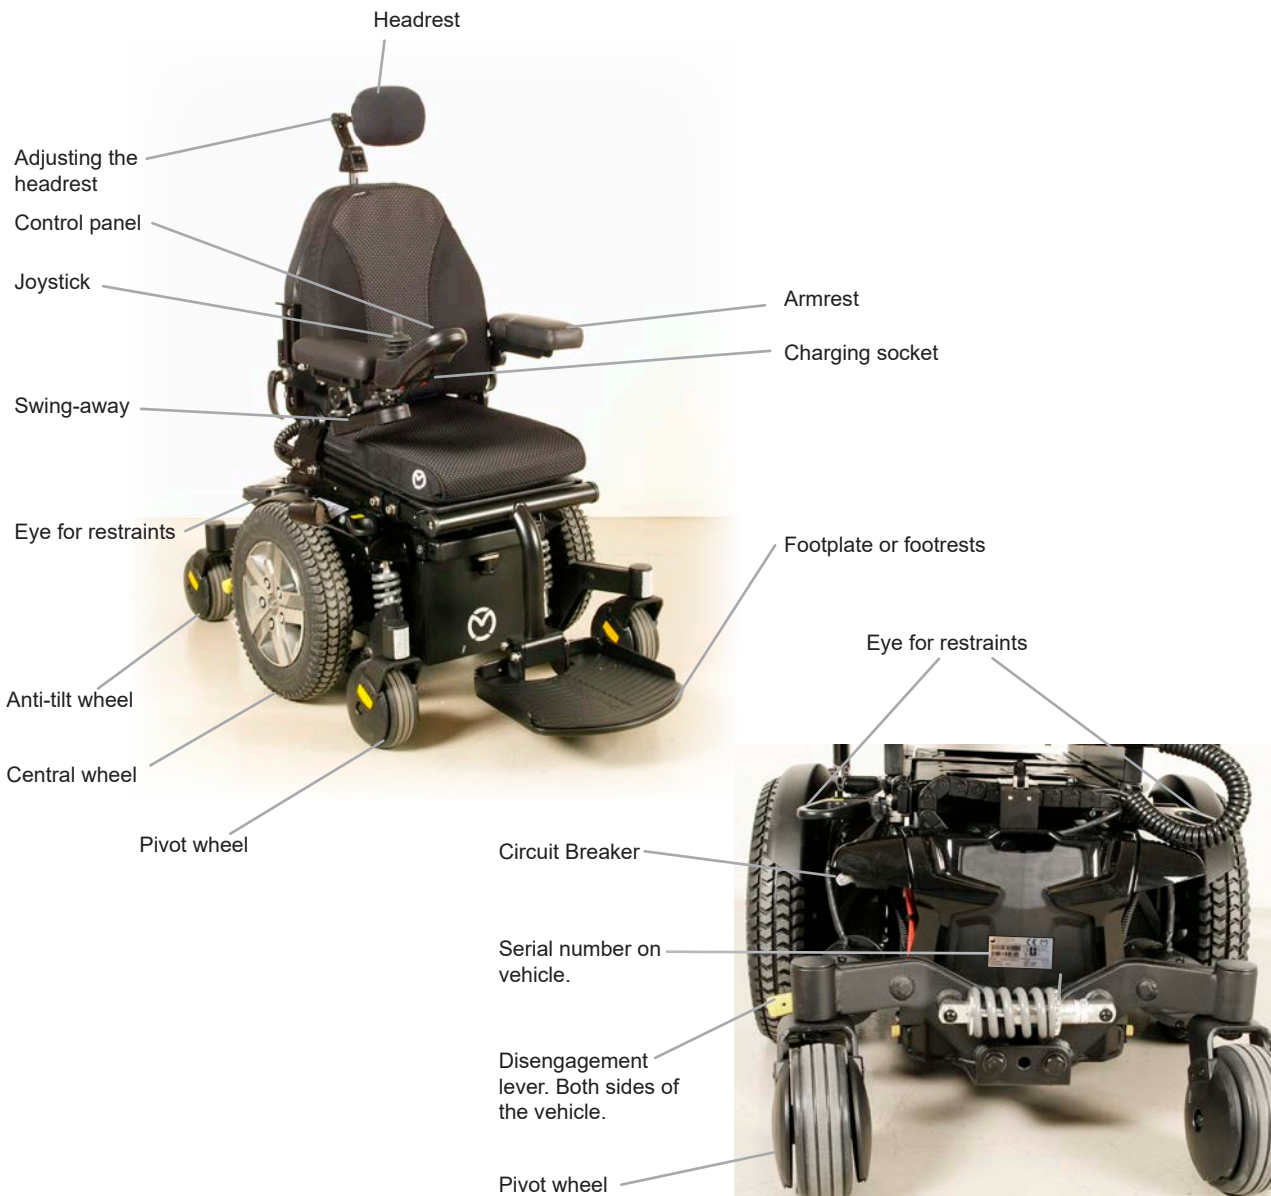

Introduction CJSM1




CJSM1 is a full programmable module based controller system, that makes it possible for the user to fully control movement and speed.














Designations - buttons

CJSM1		
	1	Start/stop-button
	2	Indicator right
	3	Function button
	4	Set up / change profile
	5	Horn
	6	Joystick
	7	Speed decrease
	8	Speed increase
	9	Light
	10	Indicator left
	11	Warning LED
	12	LCD screen

Symboles


At the top of the display you will find the status bar. Battery indicator is displayed constantly. The clock can be turned on or off as you wish. The other is lit when the corresponding function is activ.

	
	<p>Battery indicator Red, yellow and green (All bars) = Fully charged Red and yellow (Bar 1-7) = Ok, but charge when possible. Red (Felt 1-3) Steady light or slowly blinking = Charge now! Warning! Do not try to operate the chair, when the battery is almost empty. It can leave user stranded in an unsafe situation, as in the middle of the road.</p>
	<p>Time is shown as digitals in the top left corner.</p>

	Speed indicator. Tells the instantaneous speed (km / h)
1	Active profile =1
Indoor-Drive	Profile text. Shows the name of the active profile.
	When the control system contains more than one method of direct control, such as secondary joystick module or a Dual attendant module, this icon will show on the active / in charge control module.
	If the speed of the wheelchair is being limited; for example, by a raised seat, then this orange turtle symbol will be displayed.
	When the control system is operating in a latched condition this symbol will be displayed.
	The system need to restart.
	The control system have detected an error, but it is not severe enough to cause the system to trip.
	The control system has intentionally reduced the power to the motors, in order to protect them against heat damage.
	the control system has intentionally reduced its own power, in order to protect itself against heat damage.
	the control system is changing between different states. An example would be entering into Programming Mode. (Only for service technicians)
E-Stop 	If the External Profile Switch is activated during drive, or actuator operation, this symbol will be displayed.
	When Blue tooth Mode is entered the following screen will be displayed.
	If you operate the Joystick before or just after you switch the control system on, the screen will flash the joystick displaced screen. You must release and centre the Joystick to resume normal operation. If you do not release the Joystick within five seconds the wheelchair will not be able to move, even if you release the Joystick and operate it again. The screen will display a diagnostic screen at this time. You can reset this condition by switching the control system off and on again.
	This symbol will be displayed for a short time before the R-net enters into a sleep state.

Settings menu

Set Time

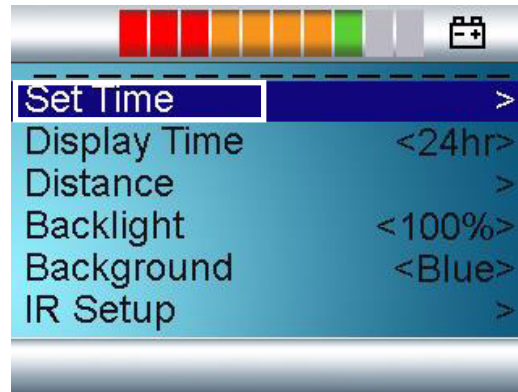


The menu is accessed by depressing the Speed Down and Speed Up buttons simultaneously (Pos 7 and 8 in the table Designations - buttons).



A right joystick deflection will enter a clock adjustment screen in which further joystick deflections are used to set the time.

Choose Exit to save and return to the main screen.



Set Display Time

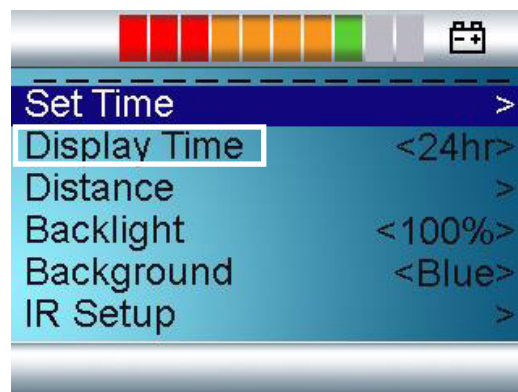

Choose the menu Display Time with the joystick. A right joystick deflection, enter the menu.

The following possibilities appears: 12hr, 24hr or OFF.
Deflect the joystick to the right /left to choose the menu you want. Choose Exit

Set Distance

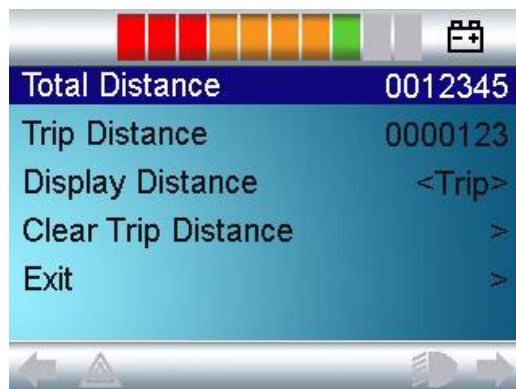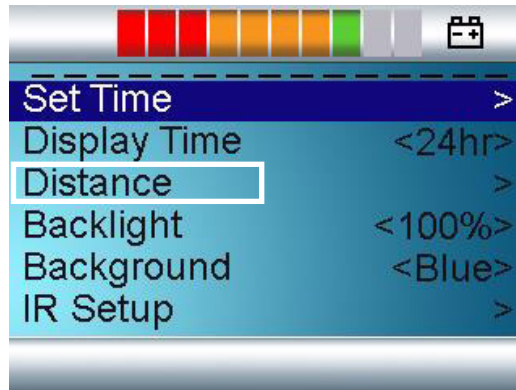

This sets the functionality of the odometer and a screen as below will appear.

Total Distance show the total distance this chair has driven with this Power module.


Trip Distance show the distance driven since last reset.

Select in this menu which value to show on the main screen.

The menu, Clear Trip Distance, resets the Trip distance to zero.


Exit - return to previous menu.

Set Backlight

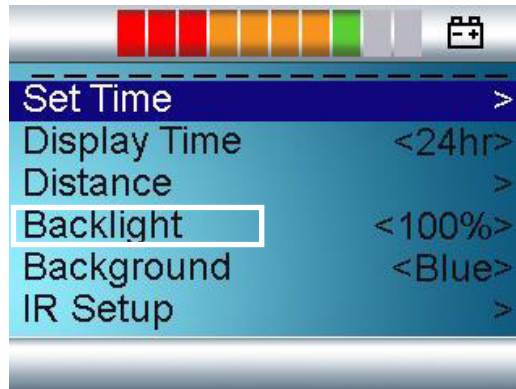

This sets the intensity of the LCD backlight. The adjustable range is 0% to 100% in steps of 10%. Adjustments are made with left and right joystick deflections.

Set Background

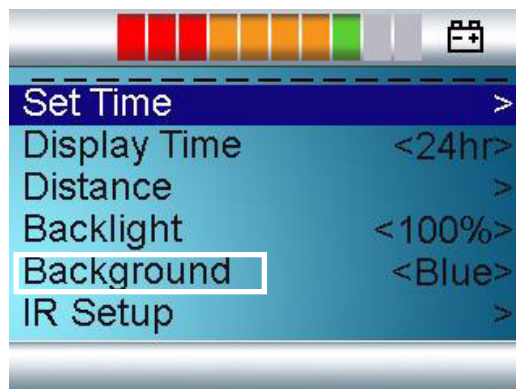

The standard setting from the factory is blue. But in bright sunlight, the white background can be better.

Options are: Blue, White, Auto.

If the choice is blue, it means that the background is blue in all profiles.

If the choice is white, it means that the background is white in all profiles.

If the choice is auto the background is controlled by the parameter Background, where the background can be set per profile a.e. Blue for Indoor use, and White for outdoor profile.

Infra red







For full details on how to learn, delete and use the IR functions available please contact Medema A/S.

Exit

Leave Settings and go back to normal use by choosing Exit.

Adjusting seat and footrest

Turn on the joystick and press the Function button (Mode) Use the joystick left/right to select the function you want to adjust. Press the joystick up/down to adjust.

Function	Icon
Tilt	
Seatback angle	
Seat lift	
Left leg support	
Right leg support	
Footrests both	

Only the available settings will be displayed.

System lock

Locking the system



Press and hold the ON/OFF button down for four seconds while the system is ON. Push the joystick forward until you hear a beep. Push the joystick back until you hear a beep. Now the system is locked.

Unlock the system



Push the joystick forward until you hear a beep. Push the joystick back until you hear a beep. Let go of the joystick. The system starts in normal mode.

Trouble shooting

If a system trip occurs, you can find out what has happened by counting the number of LEDs on the battery gauge that are flashing.

Below is a list of self-help actions. Try to use this list before you contact your service agent.

LED	Meaning
1 LED	The battery needs charging or there is a bad connection to the battery. Check the connections to the battery. If the connections are good, try charging the battery.
2 LED	The left hand motor has a bad connection. Check the connections to the left hand motor.
3 LED	The left hand motor has a short circuit to a battery connection. Contact your service agent.
4 LED	The right hand motor has a bad connection. Check the connections to the right hand motor.
5 LED	The right hand motor has a short circuit to a battery connection. Contact your service agent.
6 LED	The wheelchair is being prevented from driving by an external signal. The exact cause will depend on the type of wheelchair you have.
7 LED	A joystick fault is indicated. Make sure that the joystick is in the centre position before switching on the control system.
8 LED	A possible control system fault is indicated. Make sure that all connections are secure.
9 LED	The parking brakes have a bad connection. Check the parking brake and motor connections. Make sure the control system connections are secure.
10 LED	An excessive voltage has been applied to the control system. This is usually caused by a poor battery connection. Check the battery connections.
7 LED+ S	A communication fault is indicated. Make sure that the joystick cable is securely connected and not damaged.

Safety check

Daily safety check:

The electronic system has an integrated safety check which runs up to 100 times per minute. To supplement this check, you should carry out the following regular checks.

- Switch off the electronic system (no lights in the display)
- Check if the joystick is bent
- Check if the joystick is damaged in any other way
- Check that it returns to the central position when you release it

If the check reveals any problems, contact a competent service engineer before using the wheelchair again.

Weekly safety check:

Parking brake: This test must be carried out on a flat surface with at least one metre of free space around the wheelchair.

- Start the wheelchair and slowly move the joystick forward. There is a clicking sound. (The wheelchair may start to move in this setting).
- Immediately release the joystick and listen for the clicking sound, which should occur within one second.

Repeat in all directions.

- Check that the rubber bellows around the joystick is intact. This is important, as the bellows prevent moisture getting into the electronic system.
- Check that the control box is properly secured.

If the check reveals any problems, contact a competent service engineer before using the wheelchair again.

Monthly check

Check the tyre pressure at least once a month. It should be 2.4 bar.

Service

The MC 1124 is designed to stay safe to use for at least 10 years, up to a maximum of 5,000 hours, providing it has service and safety inspections every third year, which is equivalent to around 1500 operating hours. The service must be carried out either by Medema A/S or an authorised workshop.



IMPORTANT! For safety reasons it is of the utmost importance that service and safety check intervals are complied with, as this minimises the risk of brake failure and short-circuits in the wiring, which could generate heat and cause a fire.

Programming




The Dynamic electronic system is programmable so that the driving characteristics can be optimized for individual users. Programming must only be carried out by people trained in the control systems. Changing parameters incorrectly can produce driving characteristics that are dangerous for the user.

Serial number

All wheelchairs have a serial number plate showing the year of production, month and serial number. The same serial number can also be found on page two of the User Manual.

Please quote this number when making inquiries about servicing, spare parts, etc.

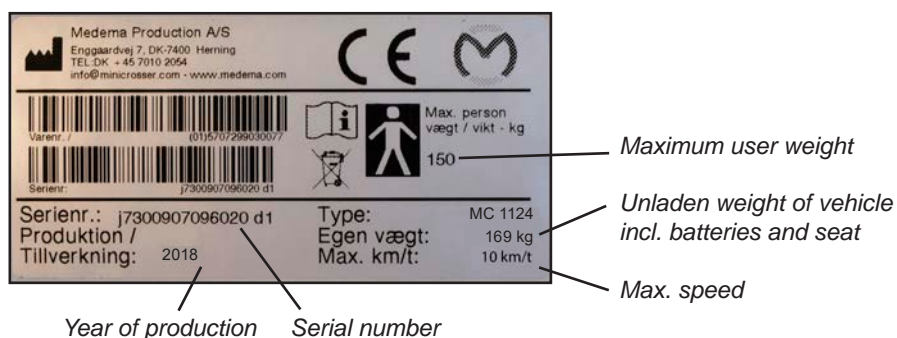

Position of serial number plate on vehicle.

Getting in and out of MC 1124

MC 1124 is a modern device, specially developed to help you achieve maximum mobility.



If you are able to move yourself to and from the electric wheelchair, follow the procedure below.

Depending on your handicap, a helper may be needed to lift you in and out of the chair.

Before entering or leaving the chair, make sure that:

- That the wheelchair is switched off.
- That the wheelchair is not disengaged.
- That the wheelchair and the seat you are moving to are both stable.
- Lift up the armrests.
- Avoid placing your full body weight on the footrests.
This may tip the wheelchair forwards. Swing the footrest to the side to leave space to stand on the floor.

Driving the MC 1124

If you are using the MC 1124 for the first time, you should try out all the day-to-day situations you are likely to encounter:

- inclines/declines,
- driving on rough terrain
- driving on sloping terrain.

You should practice these manoeuvres with your therapist or other carer.



Warning!

The seat should NEVER be hoisted while driving on uneven surfaces, slopes or up and down kerbs. The higher the seat is raised, the more unstable the chair becomes.

Arms and legs

While driving, you must place your arms on the armrests and your feet on the footrests.

Cables and leads

Always make sure that cables and leads from components like the joystick are fixed using ties.

Changes of level

Never attempt to climb onto raised objects or kerbs higher than 7 cm. Always approach changes of level head on, with the front and back wheels moving in a straight line. (See below.) This reduces the possibility of tipping.

Note!



If your MC 1124 vehicle is fitted with a docking system from Dahl Engineering, note that the clearance is reduced to 5.5 cm.



Fig. 1



Fig. 2



Fig. 3



Fig. 4

Driving on hills

When driving on hills, you should try to keep the wheelchair moving all the time. If you have to stop, start up again slowly.

When driving downhill, you must drive at the slowest speed.

If the MC 1124 starts moving faster than you want, stop it by completely releasing the joystick. Carefully push the joystick forwards again and carry on with care until you reach the bottom of the hill.



Be aware that the stopping distance can be significantly longer, down hill, than on level ground.

10 tips for driving the MC 1124:


- Reduce the speed when turning corners and going downhill.
- Reduce the speed when driving on inclines. Maximum incline: $6^\circ = 10\%$
- Reduce the speed when driving on a sideways incline. Maximum sideways incline: 6°
- Avoid parking on snow and ice.
- Always park on a level (flat) surface.
- Avoid driving on rough ground.
- Avoid driving on icy surfaces, or smooth surfaces (for example snow or freshly mown grass)
- Never attempt to climb kerbs higher than 7 cm. If the wheelchair has a docking system, the clearance is reduced to 5,5 cm.
- Avoiding driving over kerbs diagonally. There is a risk of tipping over.
- Not to be used for towing other vehicles, etc.

Note!



Talk to your doctor if you are taking medicine that may affect your ability to drive motorised vehicles.

Do not drive the MC 1124 when intoxicated. This applies to both medicine and alcohol.

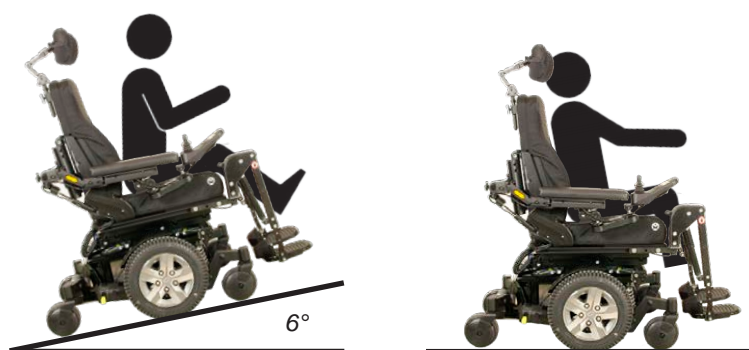

Driving on public roads:

When driving on public roads, footpaths, pedestrian streets, car parks, shopping centres, etc. you must make sure you adjust your speed and distance for other users. At 7 km/h you must follow the traffic rules applicable to cyclists. This also means that your lights must be switched on during lighting-up time. (Optional extra)

On footpaths, the maximum speed is 6 km/h. In this situation you are regarded as a pedestrian.

Note!



You should assume that other road users cannot see you while you are sitting in the MC 1124. So take great care and wait for the road to clear before crossing.



Driving on stairs/escalators:

The wheelchair is not designed for use on stairs or escalators and any attempt to do so may cause serious injury to yourself and others.

Electromagnetic compatibility (EMC)



The MC 1124 satisfies the requirements for the use of wheelchairs in an environment with electromagnetic noise. There may, however, be rare situations in which electromagnetic noise can affect the MC 1124. Sources of such noise include radio and television stations and amateur radio transmitters

If such equipment is being used close by, you are recommended to switch off the MC 1124.

If the MC 1124 starts making unintended movements, or if the brakes are released, turn the MC 1124 off as soon as it is safe to do so.

In rare cases an MC 1124 can set off shop alarms.

The control systems have been tested and meet the requirements of DS/ISO 7176-14 and DS/EN 12184.

Brakes

The MC 1124 is equipped with two sets of brakes: The motor brake and the parking brake.

Motor braking:

When you drive downhill, the control unit of the MC 1124 applies the motor brake.

Parking brake:

When the vehicle is stationary and the joystick is not moved, a magnetic brake is automatically applied to each drive unit. For driving, the magnetic brake is released first, after which the MC 1124 can be driven as described above.

Note!



You must NEVER brake the MC 1124 by switching off with the I/O button while moving, as this applies the magnetic brake with considerable force, with a resulting risk of tipping.

Disengagement:

The MC 1124 is equipped with two disengagement levers: One on each side of the vehicle.



ALWAYS disengage on both sides.

Warning!



When the wheelchair is disengaged, the braking system is deactivated. Before an occupant is left unattended or attempts to operate the wheelchair, make sure that the disengagement handles are placed in (normal position for driving), which means it's connected (the chair can not be pushed).

You must NEVER disengage on sloping terrain. This can lead to serious damage or personal injury.



Normal position for driving - pushed up



Position for disengagement - pushed down

Fuses

On the left of the MC 1124 behind the seat, there is a automatic fuse protecting the battery circuit.

The fuse is white. If it pops out, you can push it back in again after a few minutes. If it immediately pops out again, contact your authorised dealer.

The fuse can also be pulled to disconnect the power. Be aware, that you must pull it quite hard.

There are no external fuses that need to be replaced.



The automatic fuse is placed here.

Batteries

The battery indicator shows how much power is available to the wheelchair.

- Red, amber and green indicate that the batteries are fully charged.
- Red and amber indicate that the batteries will soon need recharging.
- Red indicates that the batteries need to be recharged as soon as possible, otherwise the wheelchair will cut out.

The MC 1124's batteries should be charged while not in use. This extends the service life of the batteries.

The MC 1124 is supplied with sealed, maintenance-free batteries that do not normally generate gas and do not need to be topped up with water.



Note!

Unsealed batteries must NEVER be installed in the MC 1124.

If charging is to take place outdoors, an enclosed charger without a fan should be chosen.

Only use chargers designed for charging dry maintenance-free GEL or AGM batteries.

Max. charging current 12 A.

The charging cable must NOT be extended.

New batteries can be purchased from Medema A/S.


Battery disposal

Used batteries must be disposed of through your supplier or at a recycling centre.

Take care in handling any leaky batteries, as they contain corrosive acid bound into the gel mass.

INFO: New batteries can be purchased from Medema A/S.

Charging

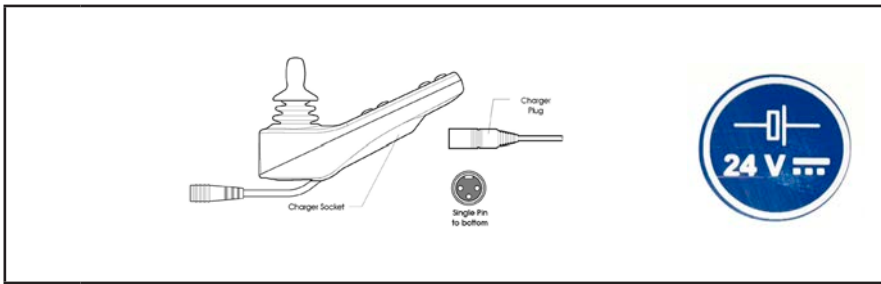

Charging	
1	Plug the cable into the control box on the wheelchair.
2	Plug the charger into the outlet or switch it on.
3	Use the indicator lights on the charger to check that charging has started.
4	When charging has finished, switch off or unplug the charger, and then remove the charger cable from the control box.

The actual battery indicator on the vehicle will show “full” after charging for a short time. However, the batteries are not fully charged until the indicator on the CHARGER turns green.

Note!

New batteries reach full capacity after approx. 20 discharge/charge cycles.

Please note that the capacity of the batteries will reduce over time and at low temperatures. Battery capacity at -10°C is half that at $+20^{\circ}\text{C}$.

If the MC 1124 is not going to be used for an extended period, charging once a month will suffice.



Note!

The charger must NOT be placed on the seat during charging.

Charging while the vehicle is switched on

- The battery indicator will flash during charging.
- After charging, the battery indicator will flash for about 1 minute after the charging cable is unplugged.

General care

If you get food or drink, etc. on the control unit, you should wipe it with a damp cloth.

You must only use a damp cloth to clean the MC 1124.



Note!

Using a high-pressure cleaner or hose may damage the wheelchair's electronic system.

Service intervals

The MC 1124 is designed to require a minimum of maintenance.

However, you are recommended to take it to your dealer for inspection every third year.



IMPORTANT! For safety reasons it is of the utmost importance that the servicing and safety check intervals are complied with, as this minimises the risk of brake failure and short-circuits in the wiring, which could generate heat and cause a fire.

(For further information see the Service Manual.)

Insurance

An MC 1124 with a maximum speed of 10 km/h is in the eyes of the law a bicycle, and no separate insurance is required.

Most contents/home insurance policies include third-party liability insurance for cyclists and so also cover MC 1124 users.

We recommend that you talk to your insurance company about this when the vehicle is delivered. If necessary, comprehensive insurance will have to be taken out separately.

Storage

The wheelchair should be stored and charged under cover, preferably at temperatures above 0°C.



Note!

The charger must be kept dry, but should not be covered when in use.

For long-term storage we recommend to disconnect the power by pulling the automatic fuse, and cover the MC 1124 to protect it from dust, rain and sunlight.

When the chair is to be used again, reconnect the automatic fuse by pushing it in, recharge the batteries completely. Check all functions.

Transporting by motor vehicle

The MC 1124 must ALWAYS be secured while being transported.

To lift the wheelchair, use the pivot wheels at the front and back. Avoid lifting by the seat or side panels.

Secure it in the vehicle with belts attached to the two eyes at the front and two at the back. All the eyes are marked in yellow.



Eyes for restraints



Important!

If your MC 1124/vehicle is fitted with a docking system from Dahl Engineering, read the instructions supplied with the docking system.

Securing to vehicle floor with belts


Dahl Engineering belt set for securing in motor vehicles.



ALWAYS use four belts at the back and two at the front.

The belts must always be attached to approved fittings in the vehicle and the four eyes welded to the MC 1124.

The belts **MUST** be attached within the angles shown in the picture for optimum safety.

The wheelchair complies with the requirements specified in DS/ISO 7176-19-2008.

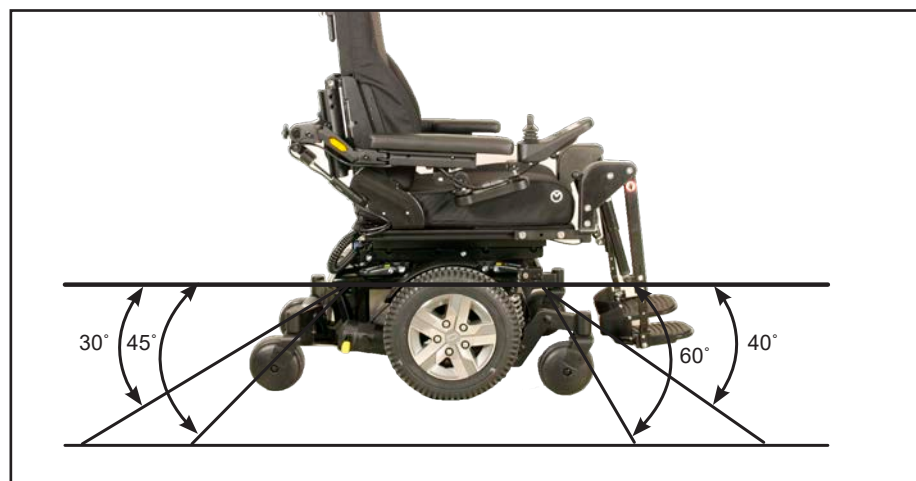

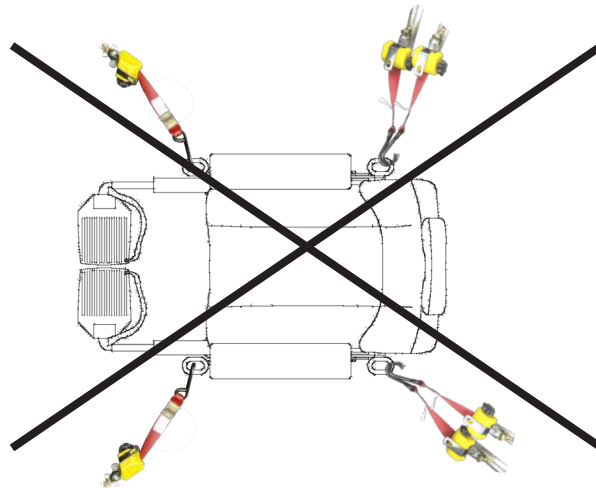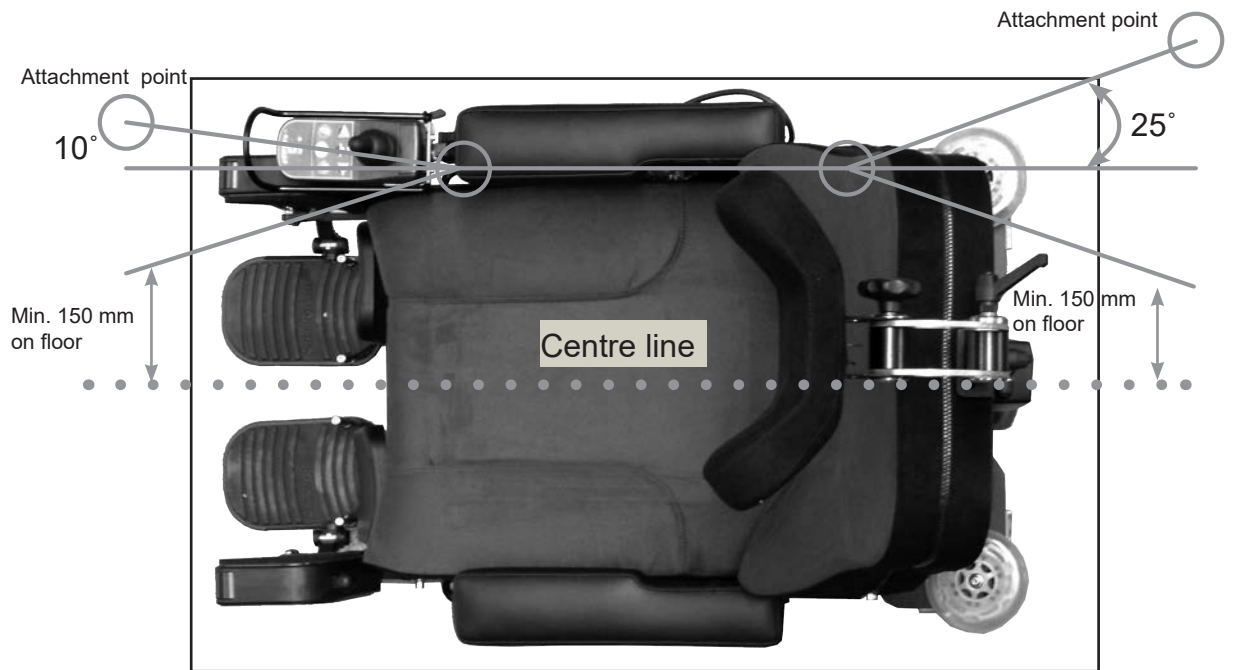

DAHL docking system

Dahl Engineering's electric Docking System sets completely new standards of flexibility and safety for wheelchair users.

The testing proved that the docking station is strong enough to cope with a load equivalent to the wheelchair weight of over 200 kg + one passenger, if the safety belt is fitted to the base of the vehicle in the traditional way.

Contact DAHL Engineering for further information and documentation.

DAHL Engineering Løvevej 3,
 DK - 7700 Thisted,
 DENMARK
 Tel. (direct) :+45 9363 5936
 Tel.: +45 96 18 00 77
 web page: wtors.com



Artikel number	Description
501750	Dahl Docking Station MK.II



Mounting the docking spear

The MC 1124 is prepared mounting of the docking spear, by predrilled holes in the chassis.

To mount the docking spear:

- Turn of the chair.
- Dismantle the legrests if mounted.
- Remove the seat
- Remove the hoist and tilt module.
- Remove the batteries.

Now the bottom of the chassis can be accessed, and the spear can be mounted.



Docking set for MC 1124



Place the nuts in the predrilled holes.



Place the screws included in the set in the spear, and mount them in the nuts.



Docking spear mounted.



As the screws are too long meaning they are higher than the nuts, they have to be adjusted. Otherwise they can ruin the batteries.

The plates in the bottom make it possible to slide the batterybox over the nuts, in and out as before.

Place the two plates on each side of the nuts. Fix them with double sided tape or a little glue.

Mount the batteries, hoist and tilt module, the seat and legrests again. Check that all functions are working ok.



The docking station is mounted in the car bottom. It must be carried out by an authorized workshop.

Move the chair over the docking station, and it will grab the spear. A click sound means it is in place and secured.


To release the chair, use the electric release button that is installed in the car in the operating area. If the car is turned off, or if it just needs power, there will be a manual release button as well.

Public transport. (Train / bus)

The wheelchair is within the requirements of external dimensions of the EU directives on public transport such as trains and buses.

Nevertheless, we recommend that free fasteners be used to fasten the chair as shown below - Fastening with seat belts to the floor.

Wheelchair users should transfer to the vehicle seat and use the vehicle-manufacturer-installed restraints systems whenever it is feasible, and the unoccupied wheelchair should be stored in a cargo area or secured in the vehicle during travel.

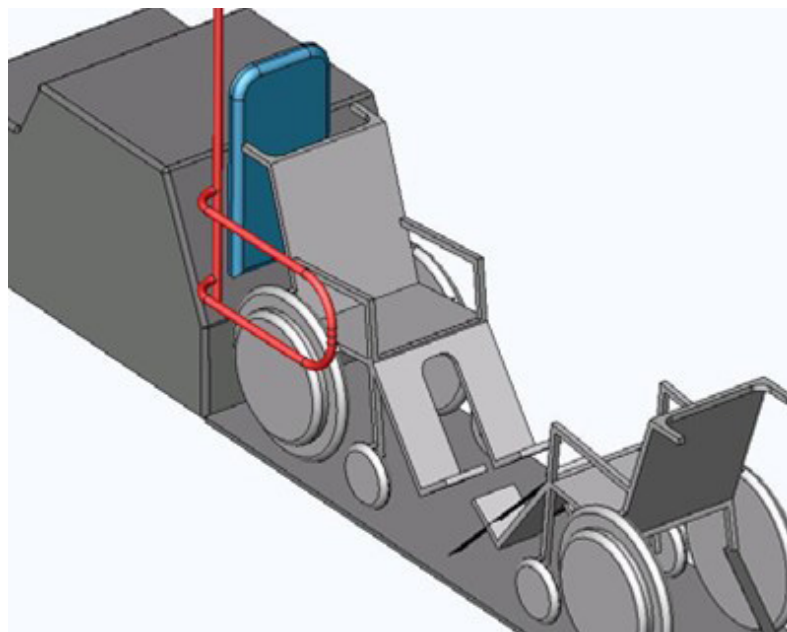

The wheelchair complies with the requirements of DS/ISO 7176-19:2008 and, as such, has been designed and tested for use only as a forward-facing seat in a motor vehicle.

Note!



Compliance with this standard does not preclude using the wheelchair facing rearward in large accessible vehicles equipped with rear-facing wheelchair passenger stations.

The wheelchair has been dynamically tested in a forward-facing orientation with the ATD restrained by both pelvic and shoulder belts (e.g. shoulder belt as part of a three-point belt restraint).

Both pelvic- and shoulder-belt restraints should be used to reduce the possibility of head and chest impacts with vehicle components.

When possible, other auxiliary wheelchair equipment should be either secured to the wheelchair or removed from the wheelchair and secured in the vehicle during travel, so that it does not break free and cause injury to vehicle occupants in the event of a collision.


Alterations or substitutions should not be made to the wheelchair securement points or to structural end frame parts or components without consulting the wheelchair manufacturer.

Spill-proof sealed batteries, such as “gelled electrolyte” should be installed on powered wheelchairs when used in a motor vehicle.

Care should be taken when applying the occupant restraint to position the seat belt buckle so that the release button will not be contracted by wheelchair components during a crash. Belt restraints must not be held away from the body by wheelchair components such as armrests or wheels.



Incorrect use of belts

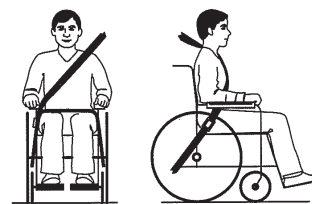

Correct use of belts

Transporting by plane

To transport the MC 1124 by plane, the airlines require:

- the batteries to be aircraft approved
- the air to be let out of the tyres
- the battery leads to be disconnected (not always, but frequently).


A main switch can be fitted (optional extra).

A battery declaration for air travel can be requisitioned from Medema A/S. See contact informations on page 2.

Towing

If you should be unfortunate enough to break down, the MC 1124 can be towed or pushed. The MC 1124 must always be turned off and disengaged for towing. See the section on Brakes.

To tow the MC 1124, secure a rope to the tow fitting on the front - marked in yellow. Do not tow faster than 5 km/h. The wheelchair will generate electricity when it is towed, with the motors acting as dynamos. If it is towed at more than 5 km/h, there is a risk of the motors generating enough electricity to damage the wheelchair and, in the worst case, cause a fire.

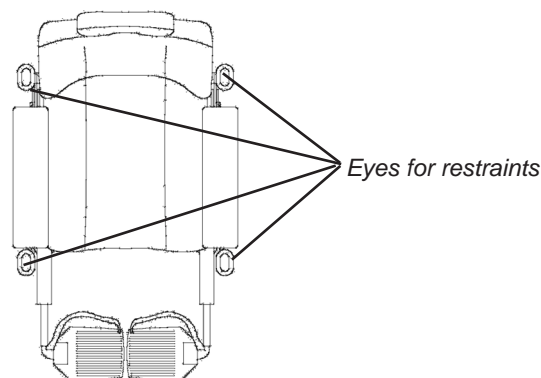

Changing the wheels

If you get a puncture in one of the pneumatic tyres or if a tyre is so badly worn that it needs to be replaced, follow the instructions below.

Tyres and inner tubes can be purchased from the authorised dealer who supplied the MC 1124.

The MC 1124 must be TURNED OFF before you start.



Jack up the MC 1124 onto a block of wood so that the wheels are clear of the floor/surface.



Central wheel

- Undo the 5 bolts.
- Take of the wheel.



Remove the valve cap and use a screwdriver or similar to open the valve to let out air.

REMEMBER!
to let all the air out before taking the wheel apart to repair a puncture.



There is a risk of explosion of the wheel, if the two rims are being taken apart with air in the tire.


Undo the rim with the 5 screws.



Replace or repair the hose.
Make sure there is no dirt or foreign objects in the tire before the the hose is in place.



Pump in some air, but don't fill it completely yet.

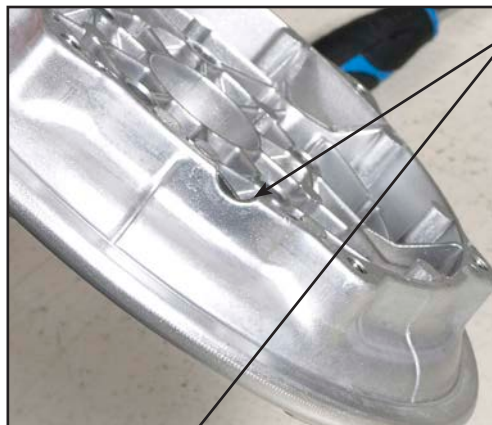

Please be aware to placing the valve in the prepared holes.





Important!

When mounting the rim, all screws must have a drop of Loctite 2400.



Mount the rim without tightening the screws.



Check that the hose doesn't get between the rim parts. Keep the rim in place while tightening the screws.

Tighten to 15 Nm



Mount the wheel back on MC 1124 again.

Tighten to 37,6 Nm



Pump the wheel to the right pressure. (see technical data)

Pivot- and anti-tilt wheel



Pivot wheel / anti-tilt wheel

Undo the central nut.

Remove the bolt that goes through the axle.



The wheel is now removable.

Checking the battery poles



Battery poles

Batteries have an approximately lifetime of two years.

Check that the cable shoes are properly mounted on the poles.


If necessary, tighten the screws.

Replacing batteries

Swing split legrests to the side, and if central footplate, adjust it in the highest possible position. Raise the seat to highest position and turn the chair off.



Pull the handle down and flip the cover out.

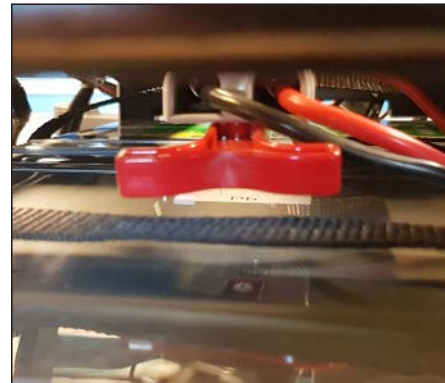


Release the plug by pulling the red handle.



Pull the battery strap to slide out the battery box.



Batteries are heavy, so be careful when you turn the box, and "drop" the batteries.

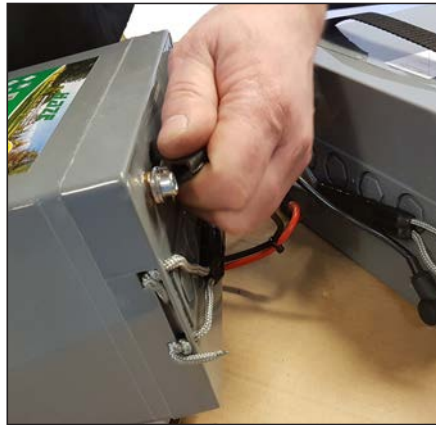

Dismantle the poles on the old batteries, and mount them on the new ones.




Place the batteries with the poles against each other.




Place the battery box on top, and turn it around.



Make sure that the plug is nearest the entrance. Slide in the battery box.

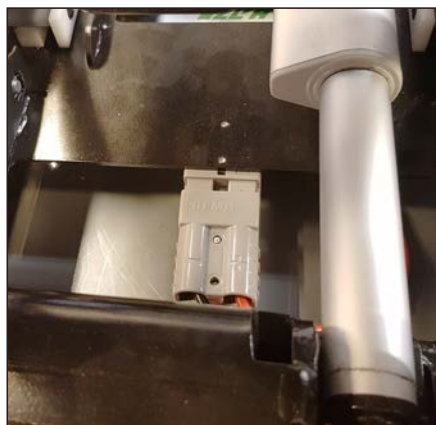

Connect the plug. Watch it from the top, and adjust /push the red handle.

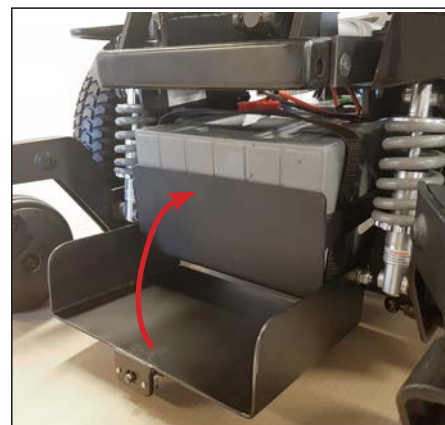

Close the cover again. Turn the chair on. Check that all functions are working ok.


Light



Light - direction

The direction of the light can be adjusted by:

- loosen the screw
- turn the lamp in the desired direction.
- tighten the screw again.

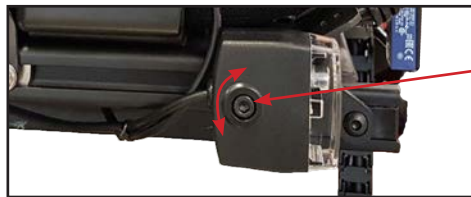

*Adjusting screw
Tool: Allen 5*



Light - located in the C-rail

The light can be moved forward/backward by:

- remove the screw/light
- disconnecting the cable if necessary.
- push the bracket in the C-rail to the position you want.
- Mount the light again.

*Adjusting screw
Tool: Allen 5*



Example - taillight

The chair is equipped with two lights in each side. Headlight and tail light.

The tail light has yellow turn signal and red tail light.

The headlight has yellow turn signal and white headlight.

Lap belt



Lap belt

If there is a need for it you can, as an accessory, mount a lap belt or harness belt on MC 1124.

The belt is designed to stay safe to use for at least 10 years.

Footplate/footrest

All the footrests are designed to stay safe to use for at least 10 years.

Manual central footplate



You can adjust the footplate forwards and back. Undo the two screws indicated on both sides.

REMEMBER to tighten again on both sides.

Gripping point when dismantling the footrest. Loosen the screws, and slide it off the rails.



To adjust the footplate to a comfortable angle for the legs, undo the screws shown here. You can now adjust the footplate.

REMEMBER to tighten the screws properly again.



To adjust the angle of the actual footplate, use the set screw under the footplate.



To adjust the footplate up and down, undo the screws shown here. You can now adjust the footplate to the required height.

REMEMBER to tighten the screws properly again.

Electric central footrest



You can adjust the footplate forwards and back. Undo the two screws indicated on both sides.

REMEMBER to tighten again on both sides.

To dismantle, loosen the two screws, and slide the footrest of the rails.



Centring the footplate: Undo the screws on both side - centre - then tighten again.

To adjust the calf pads, undo these screws. Adjust and tighten.

Gripping points.



To adjust the footplate, use the set screw shown here



Length adjustment:
Switch to the seat functions setting by pressing the Mode button.

Toggle between the settings by deflecting the joystick left / right.

The icon for the left leg support starts flashing. Move the joystick up/down to change the length.



To adjust the angle:
Use Select button until the icon for the right leg support starts flashing. Move the joystick up/down to adjust the angle.


Adjusting both parts at once: Move the joystick to the right until both leg support icons start flashing. Move the joystick up/down to adjust.

Note!

If you are using the electric central footplate, note that there is a risk of trapping in four areas when the footplate is moving forwards and backwards. See the figure below.




Manual footrests

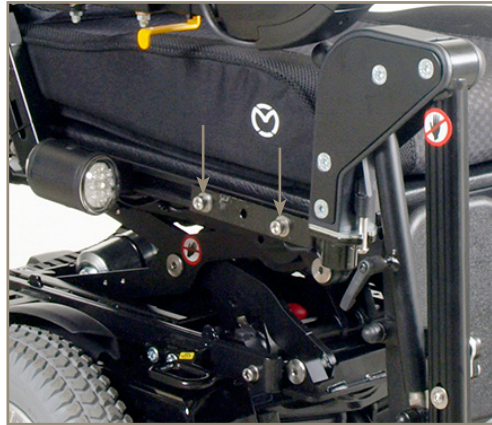

You can adjust the footrests forwards and back. This can be done by undoing the two screws indicated.

REMEMBER to tighten the screws again.

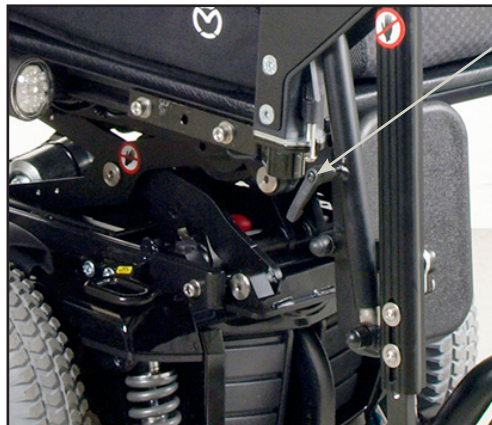

To adjust the footplate angle, loosen the clip. Adjust and tighten the clip again.



To adjust the footrests up and down, loosen these screws. Adjust and tighten the screws again.





The footrests can be swung to the side.


To do this, press your finger on the release handle. No tools are needed.



To dismantle, press the release handle. Swing the footrest out, and pull upward.

Adjusting calf pads up/down and the angle by loosening these two screws. Tighten again after adjusting.

Electric footrests

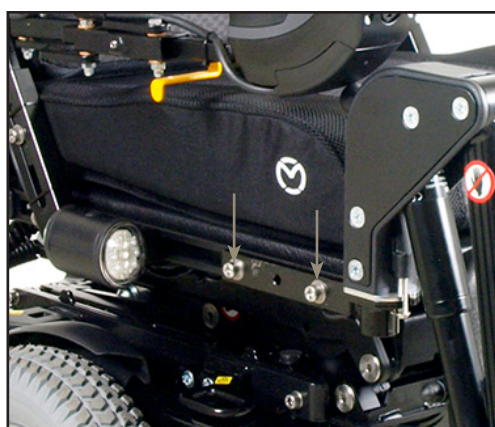

You can adjust the footrests forwards and back. This can be done by undoing the two screws indicated.

REMEMBER to tighten the screws again.



Adjusting the height and angle using the joystick:

Switch to the seat functions setting by pressing the up/down button.

Toggle between the settings by deflecting the joystick right /left.



The icon for the left leg support starts flashing, and you can adjust it by moving the joystick up and down.

Use the Select button until the icon for the right leg support starts flashing.



If both icons are flashing, you can adjust both leg supports at once.

To adjust the calf pads, undo these screws. Remember to tighten again after finishing the adjustment.




Push the release handle and swing the leg support to the side.

In this position, you will be able to lift off the leg support.

Gripping area.

Note!


There are no leads that need to be removed.

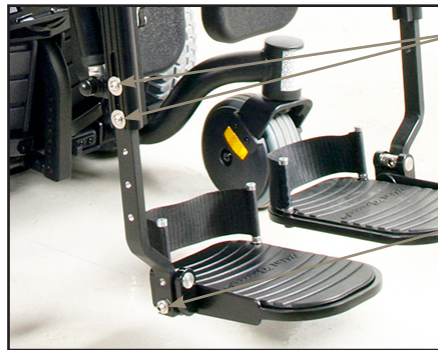

You can adjust the height manually by undoing these screws, adjusting, then tightening again.


You can adjust the angle of the footplates by undoing this screw, adjusting, then tightening again.

Electric central footrest - with split footrests

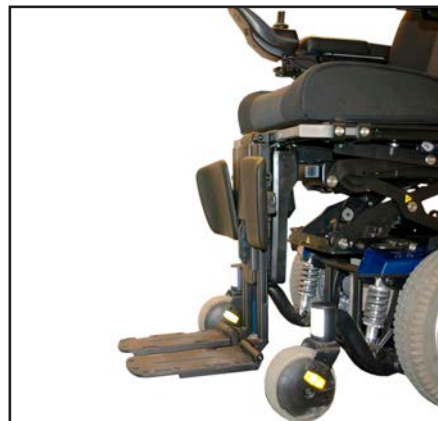

Normal start position.

Legs support vertical down.

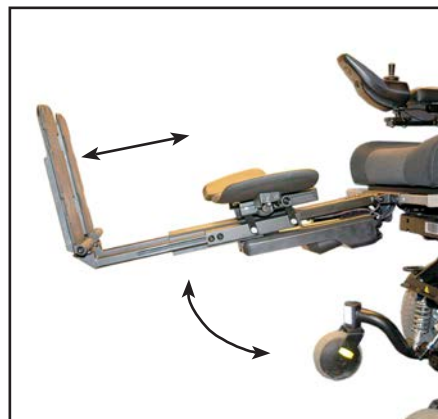

From normal start position, to the highest position, the footrest will go up with 80° and it will automatic go out in outer position, 185 mm during the cycle.



Calf pads in two different sizes




Calf pads:
Innermost position.




Calf pads:
Outermost position.

Difference of 50 mm from
the innermost to the outer-
most position

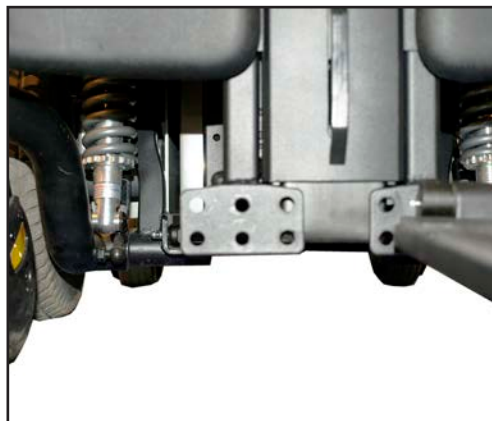


Hole pattern.
Footplate can be moved,
twice, 25 mm, on each.
(50 mm total)

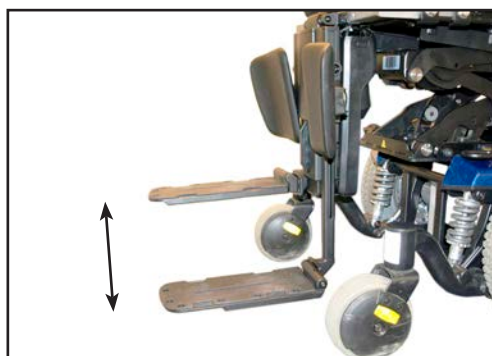

Right and left footrest,
can be adjusted manually
within a length of 160 mm



The footrests are here identical in top position

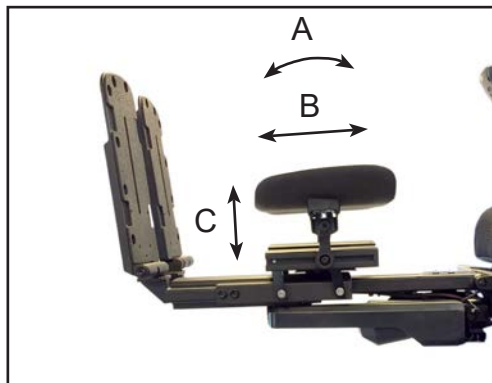


Calf pads can be moved in 3 directions.

- A Tilts
- B 130 mm
- C 50 mm



Footrests angle can be adjusted individually, using the screw as seen on the next picture.

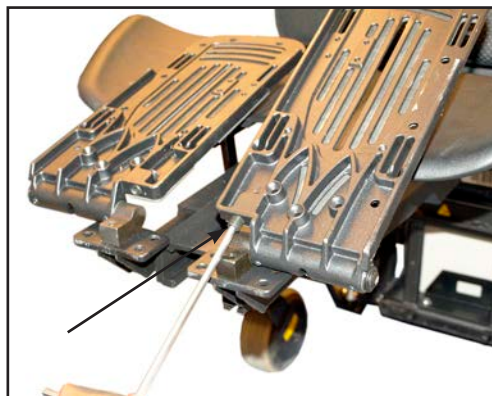

The screw as mentioned in the picture before this



Footplate.
Left and right.




Footplate with:
Width extension kit.



Footplate with:
Bell shape length extension
kit



Footplate with:
Width and length extension
kit

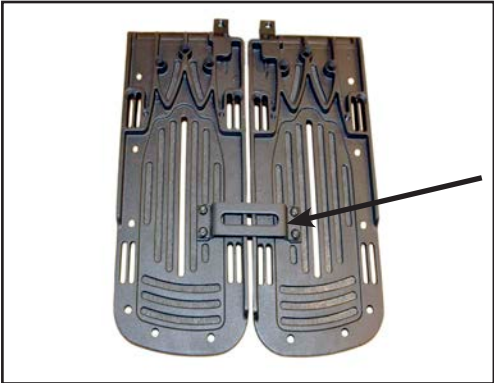


Connection of footplates:
Right and left base plate is
screwed together with the
connecting piece so that
they now act as one large
foot plate.

Adjusting the Spinalus backrest



Easy access for adjusting through these four large zippers.

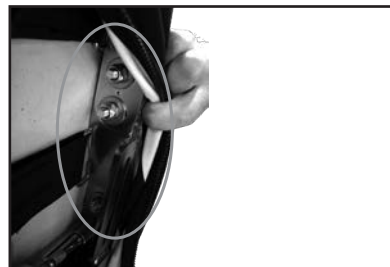


Open the zipper and find the adjustment screws




Fig. 1




Fig. 2

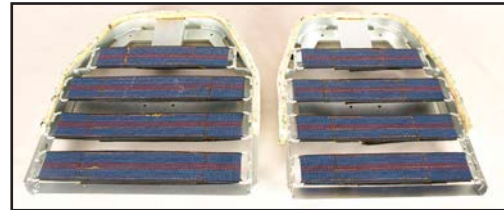

Spinalus back 30 cm and 35 cm. No adjustment possible.

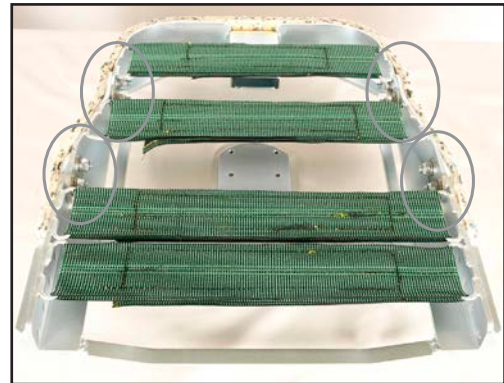

Spinalus 40 cm low. Adjustment possible in two places.

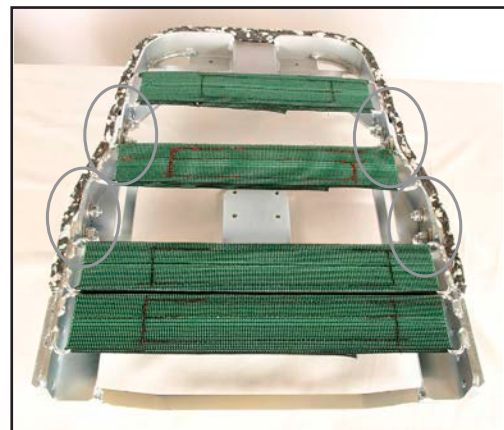

Spinalus 40 cm tall. Adjustment possible in two places.

Fig 1 og 2 shows the Spinalus-back in various positions.

Spinalus-2 settings



Spinalus-2 is designed to stay safe to use for at least 10 years


Adjusting the height of the backrest



The backrest can be adjusted up/down in several sections.

The top part of the backrest is, from the factory, mounted in the top hole. Can be moved one hole down (30 mm)

The backrest itself is, standard wise, mounted in the middle adjusting hole. From here it can be moved 25 mm up or down.

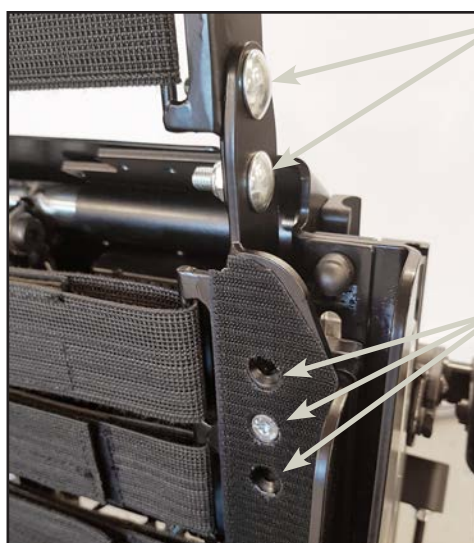

Adjusting holes for the top part of the backrest.

Tool: open end wrench
13 mm

Adjusting holes for the backrest.

Tool: Torx T30

Stepless adjustment of seat depth



Seat depth are step less adjusted between 35 and 55 cm.

Due to the construction of the back, the seat depth adjustment have no influence on the other geometry in the backrest.

At the back of the backrest is a zipper. Open the zipper

and strip the backrest cushion of from the top back frame. Pull the cushion from the velcro, fixed to the back frame. and it is free.

The seat cushion is also fixed with velcro in both sides, so lift it




off easily and remove it.

The backrest is fixed to the seat with two screws on each side.

Loosen the screws on both sides.

Tool: open end wrench 13 mm

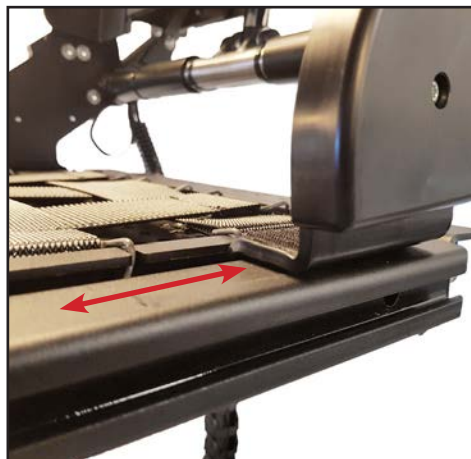

Now the backrest can be moved back/forward, to the desired position.




Height adjustment of armrest



The armrests runs in a rail, can be adjusted step less up/down. To adjust - loosen three screws. Adjust armrest - tighten the screws again.

*Loosen these screws.
Tool: open end wrench 13 mm*



Loosen these screws.



It affects the angle on the armrest, when it is adjusted up/down.

Adjust the angle by:

- Loosen these two counter nuts.
- Adjust the spindle. Screw driver in top of spindle.
- Tighten the counter nuts again.

*Tool: open end wrench 12 mm
Allen key 6 mm*

Adjusting the armrest angle in the first joint



The armrest has two joints to rotate about. We name the joints, the first and the second joint.

The second joint.

The first joint.

Tool: Allen key 6 mm



By turning the screw either one or the other way, the angle of the armrest moves in/out.

Centre of angle.



Adjusting the armrest angle in the second joint



Use the tool in the second joint, and the armrest angle moves in/out from this centre.

Tool: Allen key 6 mm



Centre of angle

By turning the screw either one or the other way, the angle of the armrest moves in/out.

Note!

When the armrest is adjusted inward, it will at some point, hit the seat.



Centre of angle

Adjusting the armrest cushion



Adjust the armrest cushion back/forward on the armrest.

- Lift up the armrest.
- Loosen the two screws.
- Adjust the armrest cushion.
- Tighten the screws again.

Tool: Torx T25

Dismantling the armrest



The armrests are fixed with a finger screw.

Loosen the finger screw.



Pull the armrest off. A new one can be mounted in reverse order.



Adjustment of the seat width



The Spinalus-2 seating system is full modular seating system from 40 to 55 cm in seat width. In steps of 5 cm.

When changing from one seat width to another, all that need to be changed, is the cushions.

Under the seat, and back cushions there is webbings

that can be adjusted for good comfort, and adjustable for varies seat widths. The upper part of the backrest, can be angled forward or backward.


The back has an adjustable dynamic recline which means that the back moves down at the same time as it is angled backwards. It is a sliding function that compensate for change of position and reduce the displacement.

The armrests follow the back and also have a dynamic movement that ensures that they are held parallel when the back is angled. The armrests are available in many different lengths and can be adjusted steplessly back and forth.

The seat depth can be adjusted steplessly from 35 to 55 cm. Due to the construction of the back, the seat depth regulation has no influence on the other geometry in the back.

Contact an authorized service technician if the width of the seat is to be changed. More information can be found in the Service Manual.

Dynamic recline

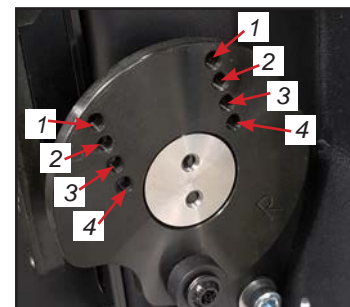

In the outer holes (hole 1) the seat back is lowered 80 mm.

You can adjust how far the seat back moves down during recline. Move the two screws (in both sides) as shown in the set of holes.

Hole	Distance
1	80 mm
2	70 mm
3	50 mm
4	40 mm

Note!



The screws must be placed similar in both sides of the seat. The closer to the centre, the screws are mounted, the less the back is lowered.

Adjusting the headrest



1 Height adjustment

2 Adjustment forward/back:

3 Headrest angle

Tool

Allen key 4 mm for adjustment

Allen key 2,5 mm for the lock

To dismantle the headrest, loosen the finger screw (pos 1) and lift of the headrest. The headrest is designed to stay safe to use for at least 10 years.

Swing-away fitting for Spinalus-2



Our Swing away fitting for Spinalus-2 have many adjustment features, to place the joystick to fit you perfectly.

The Swing away is designed to stay safe to use for at least 10 years.

Adjusting the tightness



Here you adjust how easily the Swing away should react to the push, when you need it to swing away.

Tool: Torx T10

Adjusting backward/forward on armrest



Lift up the armrest.

Two screws keep the Swing away bracket fixed to the armrest.
Loosen the screws.

Pull / push the Joystick and Swing away to the desired position. Tighten the screws again.

Tool: Allen key 5 mm

Adjusting the joystick



The Joystick bracket is attached to a ball joint. By loosen one or both screws it is possible to twist and turn the joystick to desired position.



Joystick height adjustment




By loosening this screw, the joystick can be adjusted up / down, with center in this axis.

Tool: Torx T30



Find the right location.

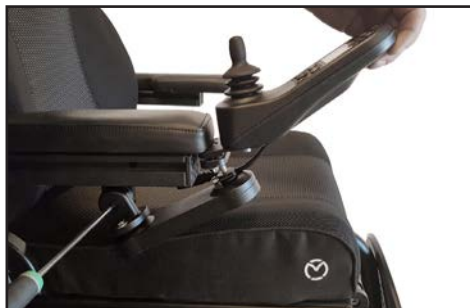

And tighten the screw again.

Tool: Torx T30



This setting also affects how far the joystick folds under the armrest.

Replace joystick



The Joystick is attached to a bracket with two screws. Remove the two screws, and unplug the plug.

Mount a new in reverse order.

Remember!
To fix the cable again with cable ties.

Tool: Allen key 4 mm

Switch joystick to opposite armrest



Remove the two screws that hold the swing away module.

Disassemble the plug.



Remove the end plug on the rail.

Let the swing away module slide off the rail.

Place it in reverse order on the other armrest.



In order to make the Swing away, swing to the other side, switch these two screws around.

Tool: Torx T25




They have different length. The longest screw should be to the right if the Swing away is mounted on the right armrest. And opposite on the left side.

Fix the cable with cable ties.

Adjusting the ION seat



Adjust the angle of the back by pulling here. Move the back to a new position. It has to click in place in both sides to be locked in place.

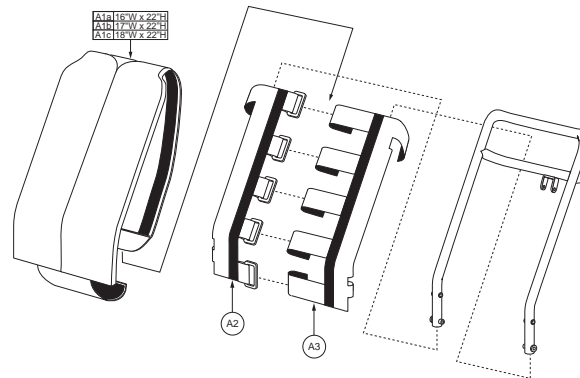

The back rest is easily adjusted with these velcro ties. The back is easy to fold for transportation.



The seat height is adjustable from 40-50 cm, by changing the mounting holes in the frame. The seat can be completed with electrical back or alternatively a gas spring.

Reconditioning

When preparing a MC 1124 for a new user it is important to check the following.

- Transaxle - clean and check for leaks. Check bearings. Check brushes in the motors.
- Tyre pressure (see technical data).
- Condition of tyres (check for cracks and abnormal wear).
- Cables (check that the cable insulation is undamaged and that no cables are trapped, secure loose cables, check for signs of heat damage).
- Control unit with joystick (check for moisture, function test).
- Batteries (load test, check battery terminals and strap).
- Charger (check that the charger is supplying the correct charge voltage/current).
- Fuses (function test).
- Moving parts like leg supports, etc. (lubricate with acid-free oil).
- Check wheels (pivot wheels, anti-tilt wheels and central wheels). Clean and check for play.
- Check the brakes/disengagement.
- Bolts and washers (check bolts/washers everywhere on the wheelchair. Check they are tightened properly and that they are intact).
- Hoist and tilt (check for breaks on the frame, hoist and tilt. Check that there are no cracks or breaks - must not be welded).
- Frame (check for cracks, remove any rust, repaint. Must not be welded).
- Switches (check the switch controlling the speed reduction when the hoist is activated).
- Accessories (check the accessories, manual and electronic. Replace any faulty finger screws or handles).
- Test drive (test all functions at their maximum settings. Test drive the wheelchair under maximum load).
- The user instructions must be provided in a plastic folder on the seat.

If the panels have lost their shine:

- Wipe the panels dry with a damp cloth.
- Wax them with car wax.

Further information: See the Service Instructions.

Returning electronic devices



Medema is certified in producer responsibility. It means that Medema collect and handle electronic waste in the category Medical equipment.

Technical data

MC 1124	
General information:	
Overall length with legrest (split legrest)	Min. 1200 mm / Max. 1720
Overall length with legrest (central legrest)	Min. 1200 mm / Max. 1720
Overall length without legrest	Min. 900 mm / Max. 900 mm
Overall width	Min. 620 mm / Max. 720 mm
Overall height (hoist lowered): (Hoist raised)	Min. 1015 mm / Max. 1095 mm Min. 1315 mm / Max. 1395 mm
Overall height incl. head rest (hoist lowered) (Hoist raised)	Min. 1155 mm / Max. 1445 mm Min. 1455 mm / Max. 1745 mm
Folded length	-
Folded width	-
Folded height	-
Total mass incl. batteries, Spinalus-2 seat (45 cm), electric leg supports, headrest, swing away and joystick.	169 kg
Total mass incl. batteries, Spinalus-2 seat (45 cm), electric central footplate adult, headrest, swing away and joystick.	174 kg
Total mass without batteries, seat, leg supports, headrest, swing away and joystick.	90 kg
Mass of the heaviest part (chassis)	65 kg
Static stability downhill	9° = 15,8%
Static stability uphill	9° = 15,8%
Static stability sideways	9° = 15,8%
Energy consumption (Distance)	Ca. 45 km (*)
Dynamic stability uphill	6° = 10,5%
Obstacle climbing	70 mm
Obstacle climbing w/spear for docking	55 mm
Maximum speed forward	10 km/h
Minimum braking distance from max. speed	2000 mm
Measured sound power level (1 m. distance)	59 db
Seat	
Seat plane angle (Spinalus-2)	Min 0° / Max 5°
Effective seat depth (Spinalus-2)	Min 350 mm / Max 550 mm
Effective seat width (Spinalus-2)	400, 450, 500, 550 mm
Hoist/tilt Raise/lower Tilt angles (***) Tilt angles optional (****)	300 mm Min -0° / Max +50° Min -5° / Max +45


MC 1124	
Seat surface height at front edge (floor to top of seat cushion) Spinalus-2 (not tilted) Standard Optional	Min 500 mm / Max 520 mm Min 465 mm / Max 485 mm
Seat surface height at front edge (floor to top of seat frame) Spinalus-2 (not tilted)	390, 430 or 450 mm
Backrest angle (Spinalus-2)	Min 0° / Max 50° (**)
Backrest height (Spinalus-2)	505 - 530 - 555 - 585 mm
Footrest to seat (top of seat cushion) distance	Min 340 mm / Max 545 mm
Leg to seat surface angle	Min 92° / 164°
Armrest to seat plate distance	Min. 180 mm / Max 320 mm
Front location of armrest structure	
Handrim diameter	-
Horizontal location of axle	Centre
Minimum turning radius without legrest	900 mm
Minimum turning radius with legrest	1200 mm
Wheel sizes: Safety wheels: front Central wheels: middle Pivot wheels: back	Ø150 mm / solid Ø350 mm / pneumatic Ø150 mm / solid
Tyre pressure for central wheels	35 psi / 2.4 bar
Motor	2 motors with central drive. 200 WK - 1200 WP
Total maximum mass of user	150 kg
ISO 7176-15 5-b the mass of the test dummy used in the test	150 kg
Suspension	Yes
Optional extras possible	Yes
Standard colour	Black
Classification	Class B
Batteries:	
Batteries	2 x 12 V / 60 Ah GEL
Battery dimensions	230 x 140 x 220 mm
Battery weight	2 x 18,5 kg
Charging time	At least 8 hours
Charger	24V DC - 10 amp
Electronic system	120 A - R-net
Lights:	
Indicators / Lights	LED



MC 1124	
The wheelchair conforms to the following standards:	
ISO 7176-15 Annex A	
a) requirements and test methods for static, impact and fatigue strengths (ISO 7176-8)	Conforms
b) Power and control systems for electric wheelchairs, requirements and test methods. (ISO 7176-14)	Conforms
c) climatic test in accordance with ISO 7176-9	Conforms
d) requirements for resistance to ignition in accordance with ISO 7176-16	Conforms
ISO 7176-19 Wheeled mobility devices for use as seats in motor vehicles.	Conforms
MC 1124 Crash tested with belts from Dahl Engineering	Passed
MC 1124 Crash tested with docking system from Dahl Engineering.	Passed

(*) Driving distance is depending on: temperature, wind, terrain, tyre pressure and user weight.



Seat angles

**

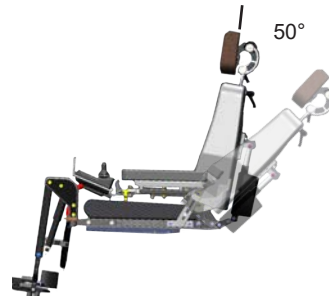

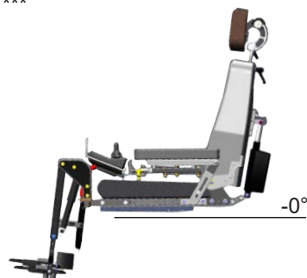

Optional





medemagroup